

Alcotest 7110 Calibration Record

Equipment

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXB-0076
Location:	SPRING LAKE POLICE		
Calibration File No.:	00156	Calib. Date:	02/21/2013
Certification File No.:	00137	Cert. Date:	08/22/2012
Linearity File No.:	00138	Lin. Date:	08/22/2012
Solution File No.:	00155	Soln. Date:	02/15/2013
Sequential File No.:	00156	File Date:	02/21/2013
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDYB S3-0001
Solution Control Lot:	12B099	Expires:	02/20/2014
		Bottle No.:	0517

Coordinator

Last Name: DENNIS

First Name: MARC

MI: W.

Signature: _____

Alcgt. [Signature]


#5925

Badge No.: 5925

Date: 02/21/2013

*Black Key Temperature Probe Serial# DDXK P2-323 *(initials)*

*Digital NIST Thermometer Serial.....# 122172162 *(initials)*

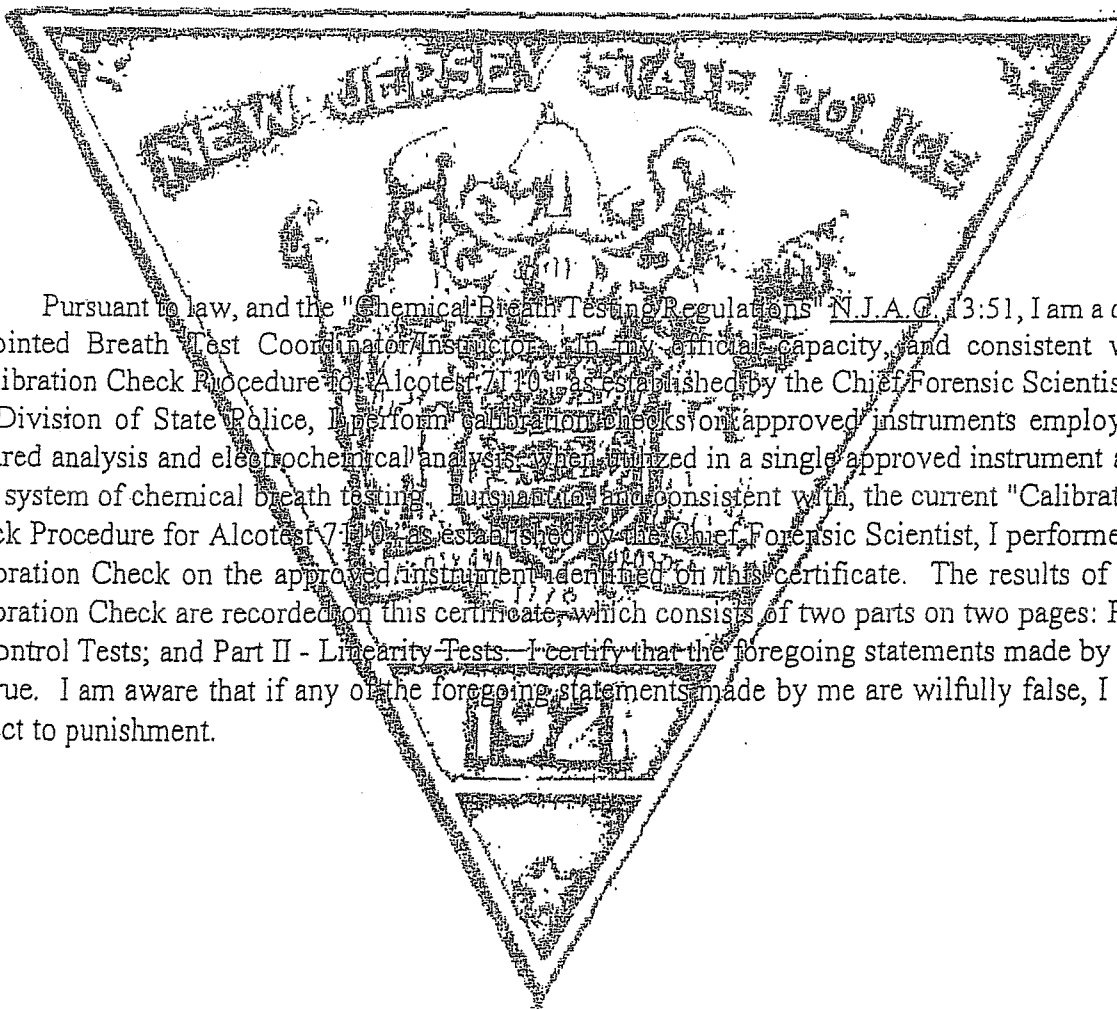

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with, the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment

Alcotest 7110 MKIII-C
Location: SPRING LAKE POLICE
Calibration File No.: 00156
Certification File No.: 00157
Linearity File No.: 00138
Solution File No.: 00155
Sequential File No.: 00157

Serial No.: ARXB-0076

Calib. Date: 02/21/2013
Cert. Date: 02/21/2013
Lin. Date: 08/22/2012
Soln. Date: 02/15/2013
File Date: 02/21/2013

Calib. No.: 00011
Cert. No.: 00010
Lin. No.: 00009
Soln. No.: 00067

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 12B099

Model No.: CU-34


Serial No.: DDYB S3-0001
Expires: 02/20/2014
Bottle No.: 0517

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:20S		
Control 1 EC	0.100%	09:21S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	09:21S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:22S		
Control 2 EC	0.098%	09:23S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	09:23S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:24S		
Control 3 EC	0.097%	09:24S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	09:24S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:25S		

All tests within acceptable tolerance.

Coordinator

Last Name: DENNIS

Signature: 

First Name: MARC

MI: W.

Badge No.: 5925

Date: 02/21/2013

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis when utilized on a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXB-0076
Location:	SPRING LAKE POLICE		
Calibration File No.:	00156	Calib. Date:	02/21/2013
Certification File No.:	00157	Cert. Date:	02/21/2013
Linearity File No.:	00158	Lin. Date:	02/21/2013
Solution File No.:	00155	Soln. Date:	02/15/2013
Sequential File No.:	00158	File Date:	02/21/2013
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.040%	Serial No.:	DDXD S3-0186
Solution Control Lot:	12H104	Expires:	08/24/2014
		Bottle No.:	0550
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.080%	Serial No.:	DDXD S3-0188
Solution Control Lot:	12H105	Expires:	08/27/2014
		Bottle No.:	0497
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.160%	Serial No.:	DDXD S3-0191
Solution Control Lot:	12I106	Expires:	09/10/2014
		Bottle No.:	1169

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:39S		
Control 1 EC	0.042%	09:39S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.040%	09:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:41S		
Control 2 EC	0.042%	09:42S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.039%	09:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:43S		
Control 3 EC	0.082%	09:44S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.079%	09:44S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:46S		
Control 4 EC	0.080%	09:46S	34.0°C	*** TEST PASSED ***
Control 4 IR	0.078%	09:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:48S		
Control 5 EC	0.159%	09:49S	33.9°C	*** TEST PASSED ***
Control 5 IR	0.159%	09:49S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:51S		
Control 6 EC	0.155%	09:51S	33.9°C	*** TEST PASSED ***
Control 6 IR	0.159%	09:51S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:53S		

All tests within acceptable tolerance.

Coordinator

Last Name: DENNIS

First Name: MARC

MI: W.

Signature: ALCO. [Signature] #5925

Badge No.: 5925

Date: 02/21/2013

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXB-0076
Location: SPRING LAKE POLICE
Calibration File No.: 00156 Calib. Date: 02/21/2013 Calib. No.: 00011
Certification File No.: 00157 Cert. Date: 02/21/2013 Cert. No.: 00010
Linearity File No.: 00158 Lin. Date: 02/21/2013 Lin. No.: 00010
Solution File No.: 00159 Soln. Date: 02/21/2013 Soln. No.: 00068
Sequential File No.: 00159 File Date: 02/21/2013

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDYB S3-0001
Control Solution %: 0.100% Expires: 11/23/2013
Solution Control Lot: 11K096 Bottle No.: 0990

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:59S		
Control 1 EC	0.101%	10:59S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:00S		
Control 2 EC	0.099%	11:01S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:01S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:02S		
Control 3 EC	0.098%	11:03S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:04S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL # DOXA P2-118 (W)

Changed By:

Last Name: DENNIS


First Name: MARC

MI: W.

Signature: ALSGT. [Signature] #5925

Badge No.: 5925

Date: 02/21/2013



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- ☒ Model: ALCOTEST® CU34
☐ Model: MARK IIA
☐ Other: _____

Serial Number:

DDXD S3-0186

Certification Date


2-6-13

Technician

BC

Re-Certification Due Date

2-6-14



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- ☒ Model: ALCOTEST® CU34
☐ Model: MARK IIA
☐ Other: _____

Serial Number:

DDXD S3-0188

Certification Date


2-5-13

Technician

BC

Re-Certification Due Date

2-5-14



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- ☒ Model: ALCOTEST® CU34
☐ Model: MARK IIA
☐ Other: _____

Serial Number:

DDXD 53-491

Certification Date

2-5-13

Technician

BC

Re-Certification Due Date

2-5-14

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDXKP2-323

Certification date:

02/05/13

Next Certification due:

02/05/14

Probe Value

103

Draeger Safety Diagnostics, Inc.
Technical Service Department

SY



Calibration
Certificate No. 1750.01

Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-4269971

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International, LLC, Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA 19087

Instrument Identification:

Model: 61220-601 S/N: 122172162 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath TC-275	A9A237		
Digital Thermometer	B16815	6/06/12	B1606038
PRT Temperature Probe	01641	5/28/12	B1526085
Temperature Calibration Bath TC-256	B01375		
Thermistor Module	A27129	10/31/12	1000306945
Temperature Probe	157	11/13/12	6-BL72N-1-1
Temperature Calibration Bath TC-179	A45240		
Thermistor Module	A17118	2/01/13	1000311439
Temperature Probe	128	2/14/13	6-BN9WZ-27-1

Certificate Information:

Technician: 68 Procedure: CAL-06 Cal Date: 3/30/12 Cal Due: 3/30/14
Test Conditions: 23.0°C 44.0 %RH 1012 mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C		N.A.		-0.000	-0.002	Y	-0.050	0.050	0.013	3.8:1
°C		N.A.		25.001	24.999	Y	24.951	25.051	0.014	3.6:1
°C		N.A.		60.000	60.000	Y	59.950	60.050	0.018	2.8:1
°C		N.A.		100.001	100.001	Y	99.951	100.051	0.018	2.8:1

This Instrument was calibrated using Instruments Traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min = As Left Nominal(Rounded) - Tolerance; Max = As Left Nominal(Rounded) + Tolerance; Date=MM/DD/YY

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Wallace Berry
Wallace Berry, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 4455 Rex Road Friendswood, TX 77546 USA
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-2006-AQ-HOU-ANAB.
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).



CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

JEFFREY S. CHIESA
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 3/20/2012

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 12B099

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1207 to 0.1211 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is February 20, 2014.

As Forensic Scientist III for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Monica L. Tramontin
Forensic Scientist III
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 22nd day of March, 2012.

Notary

MARY ELIZABETH MCLAUGHLIN
NOTARY PUBLIC OF NEW JERSEY
MY COMMISSION EXPIRES 12-24-2013



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL

DEPARTMENT OF LAW AND PUBLIC SAFETY

DIVISION OF STATE POLICE

POST OFFICE BOX 7068

WEST TRENTON, NJ 08628-0068

(609) 882-2000

CHRIS CHRISTIE

Governor

KIM GUADAGNO

Lt. Governor

JEFFREY S. CHIESA

Attorney General

COLONEL JOSEPH R. FUENTES

Superintendent

CERTIFICATION OF ANALYSIS
0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 9/26/2012

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 12H104

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0487 to 0.0491 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 24, 2014.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Ali M. Alaouie, Ph.D.

Research Scientist

NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 5th day of October, 2012.

Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL

DEPARTMENT OF LAW AND PUBLIC SAFETY

DIVISION OF STATE POLICE

POST OFFICE BOX 7068

WEST TRENTON, NJ 08628-0068

(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

JEFFREY S. CHIESA
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 9/27/2012

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 12H105

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0967 to 0.0976 grams per 100 milliliters of solution.


This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 27, 2014.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaouie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 5th day of October, 2012.

Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL

DEPARTMENT OF LAW AND PUBLIC SAFETY

DIVISION OF STATE POLICE

POST OFFICE BOX 7068

WEST TRENTON, NJ 08628-0068

(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

JEFFREY S. CHIESA
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.


ANALYSIS DATE: 10/2/2012

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 121106


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1922 to 0.1932 grams per 100 milliliters of solution.


This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 10, 2014.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

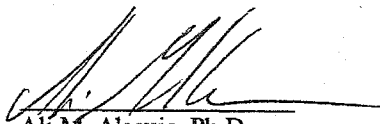
Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 5th day of October, 2012.


Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

PAULA T. DOW
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 12/16/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11K096

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1211 to 0.1217 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is November 23, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Kenneth W. Kawalek, M.S.
Assistant Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 3rd day of January, 2012.

Notary

Linda L. Desantis
Notary Public, New Jersey
My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



Dräger safety

Alcotest[®] 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:


02/21/2007

SERIAL NUMBER:

ARXB - 0076

Draeger Safety Diagnostics, Inc.
Durango, CO

CRD



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

☒ Model: ALCOTEST® CU34

☐ Model: MARK IIA

☐ Other: _____

Serial Number:

DD VB53-0001

Certification Date

Technician

Re-Certification Due Date

7-30-12

JS

7-30-13

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDXAP2-118

7-30-12

7-30-13

Probe Value

102

Draeger Safety Diagnostics, Inc.
Technical Service Department


JS


DEPARTMENT OF
Traffic and Public Safety

This is to certify that

Marc W. Dennis
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHAMPAGNE BREATHALYZER TESTS PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1946 IN THE OPERATION OF THE **Breath Test Coordinator/Instructor**
A METHOD TO DETERMINE INTOXICATION
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, 5th DAY OF November
TWO THOUSAND AND Eight


SUPERINTENDENT
NEW JERSEY STATE POLICE


ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2938 (Rev. 07/07)

DEPARTMENT OF

Traffic and Public Safety
This is to certify that
Marc W. Dennis
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1944 IN THE OPERATION OF THE **Breathalyzer**
A METHOD TO DETERMINE INTOXICATION

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS **26th** DAY OF **Sept.**
TWO THOUSAND AND **01**

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES **8/18 - 8/22/97**

Refresher Course

DATE	PLACE	INSTRUCTOR
1. 11/10/99	O.C.P.A.	Cambria
2. 11-14-04	ALTC	<i>[Signature]</i>
3. 7-17-07	ALTC	<i>[Signature]</i>
4. 10-6-05	ALTC	<i>[Signature]</i>
5. 11-18-07	OCPA	C. Potter
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

SP-293B (Rev. 4/00)

DEPARTMENT OF

Traffic and Public Safety
This is to certify that
Marc W. Dennis
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1944 IN THE OPERATION OF THE **ALCOHOL 7110 MK III-C**
A METHOD TO DETERMINE INTOXICATION

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS **30th** DAY OF **April**
TWO THOUSAND AND **Eight**

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES **12/1/2005**

Refresher Course

DATE	PLACE	INSTRUCTOR
1. 12-19-07	Ocean Co. PA	Potter
2. 3/12/09	MORRIS CO. PA	<i>[Signature]</i>
3. 2-10-11	SAYREVILLE PD	<i>[Signature]</i>
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 293B (Rev. 07/07)