

# Alcotest 7110 Calibration Record

## Equipment


Location:	Alcotest 7110 MKIII-C	Serial No.:	ARXB-0076
Calibration File No.:	SPRING LAKE POLICE		
Certification File No.:	00262	Calib. Date:	01/08/2016
Linearity File No.:	00238	Cert. Date:	07/10/2015
Solution File No.:	00239	Lin. Date:	07/10/2015
Sequential File No.:	00255	Soln. Date:	12/15/2015
	00262	File Date:	01/08/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDYB S3-0001
Solution Control Lot:	15H143	Expires:	08/17/2017
		Bottle No.:	0503

## Coordinator

Last Name:	KLIMIK	First Name:	DAVID	MI:	W
Signature:	<u>Tpr II D. Klimik #7040</u>			Badge No.:	7040
				Date:	01/08/2016

\*Black Key Temperature Probe Serial.....# DDWAP2-024 (DK)

\*Digital NIST Temperature Measuring System Serial.....# 150649679 (DK)

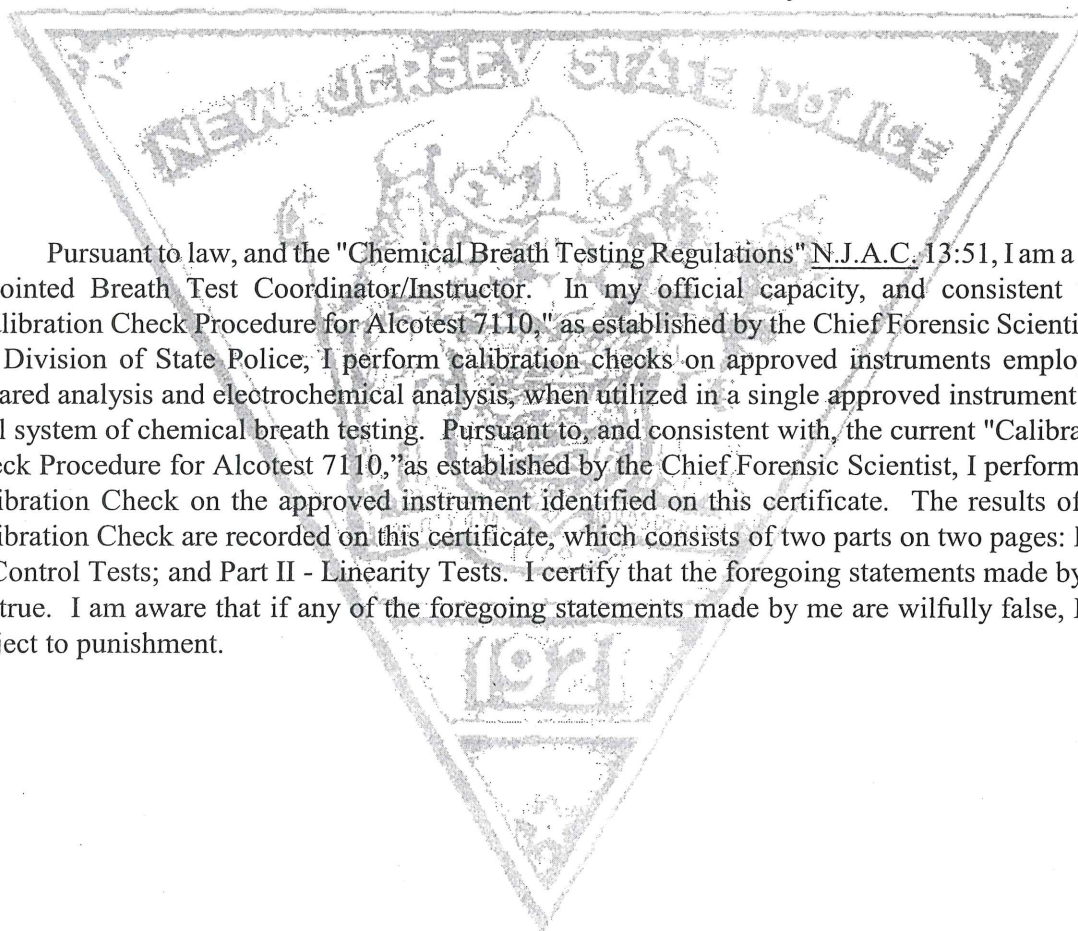

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.