

Alcotest 7110 Calibration Record

Equipment

Alcotest 7110 MKIII-C
Location: SPRING LAKE POLICE
Calibration File No.: 00685
Certification File No.: 00670
Linearity File No.: 00671
Solution File No.: 00683
Sequential File No.: 00685

Calib. Date: 12/14/2022
Cert. Date: 09/14/2022
Lin. Date: 09/14/2022
Soln. Date: 11/28/2022
File Date: 12/14/2022

Serial No.: ARXB-0076

Calib. No.: 00045
Cert. No.: 00034
Lin. No.: 00049
Soln. No.: 00257

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 21230

Model No.: CU-34

Serial No.: DDYB S3-0001
Expires: 06/23/2023
Bottle No.: 1289

Coordinator

Last Name: MIMIKOS

First Name: NICHOLAS

MI: E.

Signature: _____

TPR II. *[Signature]* #7413

Badge No.: 7413

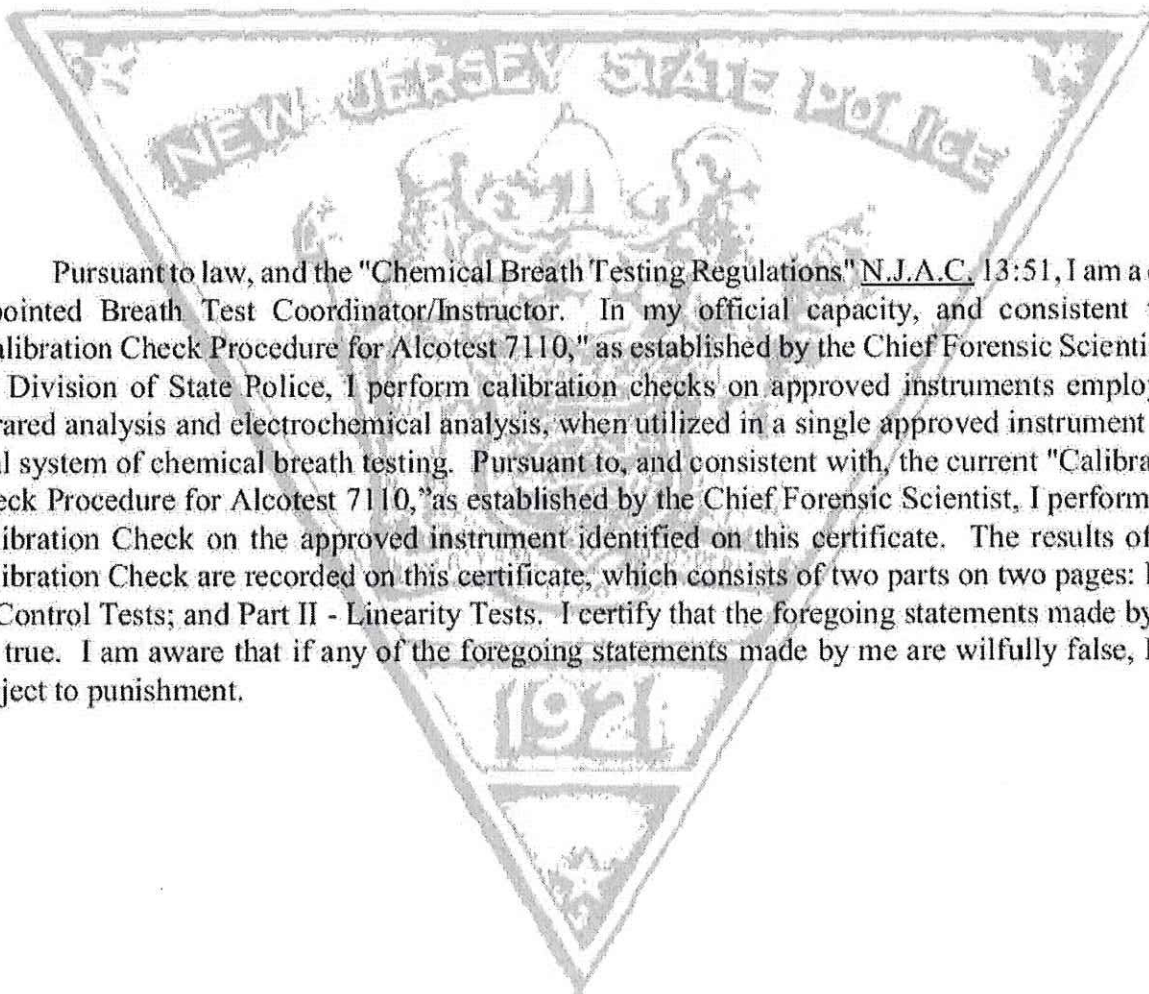
Date: 12/14/2022

*Black Key Temperature Probe Serial.....#

DDEE P2-099 (NM)

*Digital NIST Temperature Measuring System Serial.....#

210216826 (NM)



Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXB-0076
Location:	SPRING LAKE POLICE		
Calibration File No.:	00685	Calib. Date:	12/14/2022
Certification File No.:	00686	Cert. Date:	12/14/2022
Linearity File No.:	00671	Lin. Date:	09/14/2022
Solution File No.:	00683	Soln. Date:	11/28/2022
Sequential File No.:	00686	File Date:	12/14/2022
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDYB S3-0001
Solution Control Lot:	21230	Expires:	06/23/2023
		Bottle No.:	1289

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:29S		
Control 1 EC	0.099%	09:29S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:29S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:30S		
Control 2 EC	0.098%	09:31S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:31S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:31S		
Control 3 EC	0.099%	09:32S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:32S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:33S		

All tests within acceptable tolerance.

Coordinator

Last Name: MIMIKOS

First Name: NICHOLAS

MI: E.

Signature: _____

TPR II. *[Signature]* #7413

Badge No.: 7413

Date: 12/14/2022

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment

Location: Alcotest 7110 MKIII-C
SPRING LAKE POLICE
Calibration File No.: 00685
Certification File No.: 00686
Linearity File No.: 00687
Solution File No.: 00683
Sequential File No.: 00687

Calib. Date: 12/14/2022
Cert. Date: 12/14/2022
Lin. Date: 12/14/2022
Soln. Date: 11/28/2022
File Date: 12/14/2022

Serial No.: ARXB-0076

Calib. No.: 00045
Cert. No.: 00035
Lin. No.: 00050
Soln. No.: 00257

Calibrating Unit: WET
Control Solution %: 0.040%
Solution Control Lot: 21250

Model No.: CU-34

Serial No.: DDWF S3-0223
Expires: 07/06/2023
Bottle No.: 0555

Calibrating Unit: WET
Control Solution %: 0.080%
Solution Control Lot: 21260

Model No.: CU-34

Serial No.: DDXD S3-0193
Expires: 07/19/2023
Bottle No.: 1227

Calibrating Unit: WET
Control Solution %: 0.160%
Solution Control Lot: 21290

Model No.: CU-34

Serial No.: DDSC S3-0013
Expires: 07/29/2023
Bottle No.: 1188

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:42S		
Control 1 EC	0.041%	09:43S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.040%	09:43S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:44S		
Control 2 EC	0.041%	09:45S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.040%	09:45S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:46S		
Control 3 EC	0.081%	09:47S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.080%	09:47S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:48S		
Control 4 EC	0.081%	09:49S	33.9°C	*** TEST PASSED ***
Control 4 IR	0.079%	09:49S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:50S		
Control 5 EC	0.159%	09:51S	33.8°C	*** TEST PASSED ***
Control 5 IR	0.160%	09:51S	33.8°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:52S		
Control 6 EC	0.158%	09:53S	33.8°C	*** TEST PASSED ***
Control 6 IR	0.161%	09:53S	33.8°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:54S		

All tests within acceptable tolerance.

Coordinator

Last Name: MIMIKOS

First Name: NICHOLAS

MI: E.

Signature: _____

TPR II. *[Signature]* #7413

Badge No.: 7413

Date: 12/14/2022

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXB-0076
Location:	SPRING LAKE POLICE		
Calibration File No.:	00685	Calib. Date:	12/14/2022
Certification File No.:	00686	Cert. Date:	12/14/2022
Linearity File No.:	00687	Lin. Date:	12/14/2022
Solution File No.:	00688	Soln. Date:	12/14/2022
Sequential File No.:	00688	File Date:	12/14/2022
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDYB S3-0001
Solution Control Lot:	21480	Expires:	12/28/2023
		Bottle No.:	1456

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:02S		
Control 1 EC	0.100%	11:03S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:03S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:03S		
Control 2 EC	0.100%	11:04S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:04S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:05S		
Control 3 EC	0.099%	11:05S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:05S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:06S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: _____

DDXA P2-118 (NM)

Changed By:

Last Name: MIMIKOS

First Name: NICHOLAS

MI: E.

Signature: _____

APR II. A. J. #7413

Badge No.: 7413

Date: 12/14/2022

Alcotest 7110 MKIII-C Calibration
NIST-Traceable Digital Thermometer Readings

Coordinator:

TPR II. Nicholas E. Mimikos
Name

7413
Badge No.

Location:

Spring Lake Police
Agency

ARXB-0076
Alcotest Serial No.

Equipment:

210216826
Digital NIST Temperature Measuring System Serial No.

Simulator Solution Concentration	CU-34 Simulator Serial No.	Time Simulators Started to Heat	Time Temp. Reading Obtained	Temp. Reading on NIST Traceable Thermometer
0.04%	DDWF S3-0223	08:18S	09:20S	34.0°C
0.08%	DDXD S3-0193	08:18S	09:21S	33.9°C
0.10%	DDYB S3-0001	08:18S	09:23S	33.9°C
0.16%	DDSC S3-0013	08:18S	09:24S	33.8°C

Pursuant to law and the "Chemical Breath Testing Regulations" established at N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity and consistent with the "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on Alcotest 7110 MKIII-C instruments. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110", I performed a Calibration Check Procedure on the Alcotest 7110 MKIII-C instrument identified on this certificate. Pursuant to the current "Calibration Check Procedure for Alcotest 7110", I used the Digital NIST-traceable Temperature Measuring System identified on this certificate to confirm that the temperatures of the 0.10%, 0.04%, 0.08%, and 0.16% Simulator Solutions used in the respective CU-34 Simulators identified on this certificate, were 34.0 degrees Celsius \pm 0.2 degrees Celsius. I hereby certify that I truthfully recorded on this certificate the temperatures of each of the simulator solutions as shown on the Digital NIST-traceable Temperature Measuring System thermometer. I am aware that if any of the foregoing statements made by me are willfully false, I am subject to punishment.

TPR II. A. #7413
Coordinator's Signature

12/14/2022
Date

Dräger

Alcotest 7110

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for portable breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48654, 49 FR 48654, and 50 FR 48705. The manufacturer guarantees accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your state's specifications.

Certification Date:

Serial Number:

6/21/21

ARXB-0076

Dräger, Inc.

GR



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-12064542

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International LLC Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA, 19087

Instrument Identification:

Model: 61220-601,

S/N: 210216826

Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Thermistor Module	A27129	01 Mar 2022	1000464865
Temperature Calibration Bath	A45240		
Temperature Calibration Bath	A73332		
Temperature Calibration Bath	B01375		
Temperature Probe	5394	08 Mar 2022	C1228019
Temperature Calibration Bath	B3A444		
Temperature Probe	5357	09 Jun 2021	C0428083
Thermistor Module	B5C344	06 Jun 2021	1000452872
Thermistor Module	B96381	21 Aug 2021	1000457544
Temperature Probe	5392	04 Aug 2021	C0804052
Temperature Probe	5398	04 Aug 2021	C0804051

Certificate Information:

Technician: 420

Procedure: CAL-06

Cal Date: 17 Mar 2021

Cal Due Date: 17 Mar 2023

Test Conditions: 62.18%RH 22.28°C 1006mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C	N.A.	N.A.		0.000	0.000	Y	-0.05	0.05	0.0087	>4:1
°C	N.A.	N.A.		24.999	25.000	Y	24.949	25.049	0.0087	>4:1
°C	N.A.	N.A.		50.001	50.001	Y	49.951	50.051	0.0087	>4:1
°C	N.A.	N.A.		100.000	100.001	Y	99.95	100.05	0.0087	>4:1

This certificate indicates Traceability to standards provided by (NIST) National Institute of Standards and Technology and/or a National Standards Laboratory.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement": (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min=As Left Nominal(Rounded) - Tolerance; Max= As Left Nominal(Rounded) + Tolerance;

Nicol Rodriguez

Nicol Rodriguez, Quality Manager

Marisa Elms

Marisa Elms, Technical Manager

Note :

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometer change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com

Control Company is an ISO/IEC 17025:2017 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-ANAB.
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-12064542

Traceable® Certificate of Calibration for Digital Thermometer

Recalibration:

or factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

Issue Date : 17 Mar 2021

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com

Control Company is an ISO/IEC 17025:2017 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-ANAB.
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).



Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

☒ Model: ALCOTEST CU34

☐ Model: MARK IIA

☐ X-Cal 2000 (Alcosim)

☐ Other: _____

Serial Number:

DDWFS3-0223

Certification Date:

4.5.22

Technician:

MB

Re-Certification Due Date:

4.5.23



Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

☒ Model: ALCOTEST CU34

☐ Model: MARK IIA

☐ X-Cal 2000 (Alcosim)

☐ Other: _____

Serial Number:

DDXDS3-0193

Certification Date:

4.1.22

Technician:

MB

Re-Certification Due Date:

4.1.23

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

☒ Model: ALCOTEST CU34

☐ Model: MARK IIA

☐ X-Cal 2000 (Alcosim)

☐ Other: _____

Serial Number:

DDSCS3-0013

Certification Date:

4.5.22

Technician:

MB

Re-Certification Due Date:

4.5.23

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDEEP2-099

Certification Date:

4.1.22

Next Certification Due:

4.1.23

Probe Value:

105

Dräger, Inc.

MB

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249, 12/19/94 Notices)
Dräger, Inc.

☒ Model: ALCOTEST CU34

☐ Model: MARK IIA

☐ X-Cal 2000 (Alcosim)

☐ Other: _____

Serial Number:

DDYB53-0001

Certification Date:

5-20-22

Technician:

MB

Re-Certification Due Date:

5-20-23

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into this Alcotest 7110.

Serial Number Temp Probe:

DDXAP2-118

Certification Date:

5-20-22

Next Certification Due:

5-20-23

Probe Value:

103

Dräger, Inc.

MB



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS 0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 07/08/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21230

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1200 to 0.1218 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 23, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 20 day of July, 2021.
[Signature]
Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURDIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS 0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 07/27/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21250

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0485 to 0.0489 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 06, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28 day of July, 2021.
[Signature]
Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110622
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS **0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.


ANALYSIS DATE: 07/27/2021


BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21260

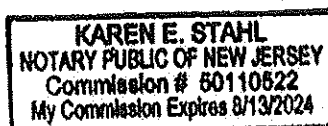
Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0970 to 0.0977 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 19, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28 day of July, 2021.

Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

ANDREW J. BRUCK
Acting Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS **0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.


ANALYSIS DATE: 08/11/2021


BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21290

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1945 to 0.1977 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 29, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 20 day of August, 2021.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110522
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

ANDREW J. BRUCK
Acting Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS **0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.


ANALYSIS DATE: 01/12/2022

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21480

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1208 to 0.1227 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is December 28, 2023.

As Acting OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.



Michael Kennedy
Acting OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 19 day of January, 2022.


Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110822
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



DEPARTMENT OF
Law and Public Safety
This is to certify that

NICHOLAS E. MIMIKOS
NEW JERSEY STATE POLICE

IS QUALIFIED AND COMPETENT TO CONDUCT OPERATIONAL BREATH ANALYSIS PURSUANT TO CHAPTER 143 OF
THE LAWS OF 1966 IN THE OPERATION OF THE **ALCOTEST 7110 MKIII-C**
A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 23rd DAY OF **OCTOBER**

TWO THOUSAND AND **FOURTEEN**

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 6-3-16	Berlen C.P.A.	<i>[Signature]</i>
2. 1-19-18	Berlen C.P.A.	<i>[Signature]</i>
3. 2-20-20	Berlen C.P.A.	<i>[Signature]</i>
4. 7/25/22	Lakehurst	<i>[Signature]</i>
5.		
6.		
7.		
8.		
9.		

S.P. 2838 (Rev. 08/13)

DEPARTMENT OF
Law and Public Safety
This is to certify that

Nicholas E. Mimikos
Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT OPERATIONAL BREATH ANALYSIS PURSUANT TO CHAPTER 143 OF
THE LAWS OF 1966 IN THE OPERATION OF THE **Alcotest 7110 MKIII-C**
A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 9th DAY OF **October**

TWO THOUSAND AND **Eighteen**

[Signature]
COLONEL
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2838 (Rev. 01/14)